



Anti-CENP-B ELISA Kit

Catalog Number EA-5008

(For Research Use Only)

Introduction

Anti-centromere antibodies (ACA) are an immunological marker for diagnosis of CREST syndrome, a limited form of systemic sclerosis. At least 9 proteins are known to be associated with the centromere complex, but CENP-B is normally considered to be the major centromere antigen. CENP-B has a molecular weight of approximately 66 kDa and plays an important role in the formation of the centromeric chromatin. CENP-B antibodies are present in the sera of up to 80% of patients with CREST syndrome. These autoantibodies are also often detected in sera from patients with Raynaud's phenomenon and occasionally in other rheumatic diseases such as systemic lupus erythematosus, Sjögren's syndrome, and rheumatoid arthritis. ACA have also been reported to occur with high prevalence in patients with primary biliary cirrhosis, in patients with malignancies and occasionally in normal individuals.

Principle of the assay

Anti-CENP-B ELISA kit measures anti-CENP-B antibodies in the serum. It is based on the principle of a solid phase enzyme-linked immunosorbent assay. The assay utilizes CENP-B protein for immobilization on the microtiter wells and anti-human IgG antibodies conjugated to horseradish peroxidase (HRP) for detection. The test sample is allowed to react simultaneously with the two components, resulting in anti-CENP-B antibodies being sandwiched between the solid phase and enzyme-linked antibodies. After incubation, the wells are washed to remove unbound-labeled antibodies. A HRP substrate, TMB, is added to result in the development of a blue color. The color development is then stopped with the addition of Stop Solution changing the color to yellow. The concentration of anti-CENP-B is directly proportional to the color intensity of the test sample. Absorbance is measured spectrophotometrically at 450 nm.

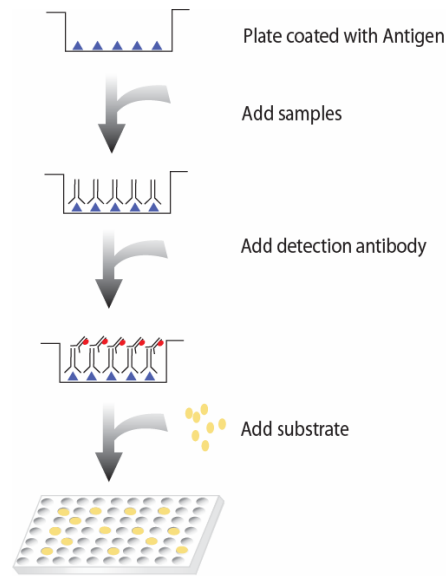


Diagram of ELISA

Materials provided with the kit

- 96-well plate coated with CENP-B (4°C).
- Anti-human IgG antibody conjugated to HRP (4°C).
- 1X Diluent buffer (4°C).
- 5X Assay wash buffer (4°C).
- Substrate (4°C).
- Stop Solution (4°C)

Material required but not provided

- Microplate reader capable of measuring absorbance at 450 nm
- Shaker

Reagent preparation before starting experiment

- Dilute the 5x Assay wash buffer to 1x buffer
40ml 5x Assay wash buffer
160ml ddH₂O
- Dilute 1000 times of anti-human IgG antibody conjugated to HRP with 1X Diluent buffer.

Storage and Preparation

Store all reagents at 2-8°C.

All reagents must be brought to room temperature (20-25°C) prior to use.

When stored at 2-8°C, the diluted Assay wash buffer is stable until the kit expiration date.

Precautions

Human blood derivatives and patient specimens should be considered potentially infectious. All human derived components need to be tested for the negative HBsAg, HCV, HIV-1 and 2 and HTLV-I. Follow good laboratory practices in storing, dispensing and disposing of these materials.

Assay procedure

1. Cut the sealing film over the plate and remove it from the desired number of well strips. Make sure the rest of wells are well sealed.
2. Add 100 μ l of diluted samples (1:100 diluted or further 2 serial diluted serum) per well and incubate for 1 hour at room temperature with gentle shaking.
3. Aspirate each well and wash by adding 200 μ l of 1X Assay wash buffer. Repeat the process twice for a total of three washes. Completely remove liquid at each wash by firmly tapping the plate against clean paper towels.
4. Add 100 μ l of diluted anti-human IgG antibody conjugated to HRP to each well and incubate for 0.5 hours at room temperature with gentle shaking.
5. Repeat the aspiration/wash as in step 3.
6. Add 100 μ l of Substrate to each well and incubate for 5-30 minutes.
7. Add 50 μ l of Stop solution to each well. The color in the wells should change from blue to yellow.
8. Determine the optical density of each well with a microplate reader at 450 nm within 30 minutes.

Example

