

# Human IP-10 ELISA

Catalog Number EA-0505

### Introduction

IFN-gamma-inducible protein (IP-10) is a member of the chemokine family of cytokines and is induced in a variety of cells in response to interferon gamma and lipopolysaccharide. It is secreted by a number of cells including monocytes, endothelial cells and fibroblasts. IP-10 plays several roles, such as chemoattraction for monocytes/macrophages, T cells, NK cells, and dendritic cells, promotion of T cell adhesion to endothelial cells, antitumor activity, and inhibition of bone marrow colony formation. several cell types in response to IFN- $\gamma$ . IP-10 acts as potent inhibitors of angiogenesis in vivo.

# Principle of the assay

IP-10 ELISA is based on the principle of a solid phase enzyme-linked immunosorbent assay. The assay utilizes rabbit anti-human IP-10 for immobilization on the microtiter wells and biotinylated rabbit anti-human IP-10 antibodies along with streptavidin conjugated to horseradish peroxidase (HRP) for detection. The test sample can react simultaneously with the two antibodies, resulting in the IP-10 molecules being sandwiched between the solid phase and enzyme-linked antibodies. After incubation, the wells are washed to remove unbound-labeled antibodies. An HRP substrate, TMB, is added to result in the development of a blue color. The color development is then stopped with the addition of Stop Solution changing the color to yellow. The concentration of IP-10 is directly proportional to the color intensity of the test sample. Absorbance is measured spectrophotometrically at 450 nm.

(For Research Use Only)

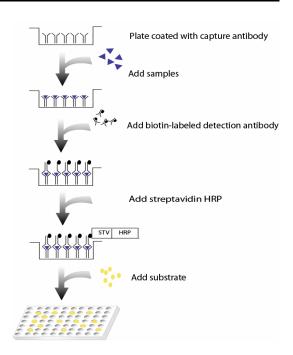


Diagram of ELISA

# Materials provided with the kit

Component	Qty	Store at
8x12 96-Well 12 strip Plate	1	4°C
coated with rabbit anti-		
human IP-10 antibodies		
Biotin labeled rabbit anti-	25 µL	-20°C
human IP-10 antibodies		
Human IP-10 protein	10 µL	-20°C
standard (200ng/ml)		
Streptavidin-HRP conjugate	50 µL	4°C
1xDiluent buffer	40 mL	4°C
5X Assay wash buffer	40 mL	4°C
Substrate	10 mL	4°C
Stop solution	5 mL	4°C

### Material required but not provided

- Microplate reader capable of measuring absorbance at 450 nm
- Deionized or distilled water.


# **Reagent preparation before starting** experiment

- Dilute the 5x Assay wash buffer to 1x buffer . 40 ml 5x Assay wash buffer 160 ml ddH2O
- Use serum-free conditioned media or original or 10-• fold diluted sera. Sera can be diluted with 1X Diluent buffer. When serum-containing conditioned media is required, be sure to use serum as a control.
- Dilute 50 times of human IP-10 protein standard • (200 ng/ml) with 1X Diluent buffer to 4000 pg/ml and then do a 2-fold serial dilutions by adding 4 ul of the diluted Human IP-10 protein standard in 200 ul 1X Diluent Buffer (See Step 2 below for detailed instruction).
- Dilute 400 times of biotin labeled rabbit anti-human IP-10 antibodies with 1X Diluent buffer before use.
- Dilute 200 times of streptavidin-HRP with 1X Diluent buffer before use.

### Assay procedure

1. Calculate the number of samples to decide how many strips need to be used.

2. Add 100 µl of Standard, control, or sample per well and incubate for 1 hour at room temperature with gentle shaking.



(See picture) Incubate each well for 1 hr at room temperature with gentle 3. Aspirate each well and wash by adding 200 µl of 1X

Assay wash buffer. Repeat the process three times for a total of three washes. Completely remove liquid at each wash. After the last wash, remove any remaining liquid by inverting the plate against clean paper towels.

4. Add 100 µl of diluted biotin-labeled rabbit anti-human IP-10 antibodies to each well and incubate for 1 hour at room temperature with gentle shaking.

5. Repeat the aspiration/wash as in step 3.

6. Add 100 µl of diluted streptavidin-HRP conjugate to each well and incubate for 45 min at room temperature with gentle shaking.

- 7. Repeat the aspiration/wash as in step 3.
- 8. Add 100 ul of substrate to each well and incubate for 5-30 minutes.

9. Add 50 µl of Stop solution to each well. The color in the wells should change from blue to yellow.

10. Determine the optical density of each well with a microplate reader at 450 nm within 30 minutes.

#### **Example of standard curve**

